



LEEDS  
BECKETT  
UNIVERSITY

---

Citation:

Clarkson, S and Flint, SW and Broom, DR and Capehorn, M and Wheat, J (2018) 3D surface-imaging for volumetric measurement in people with obesity. *Technology and Health Care*, 26 (2). pp. 363-369. ISSN 0928-7329 DOI: <https://doi.org/10.3233/THC-171138>

Link to Leeds Beckett Repository record:

<https://eprints.leedsbeckett.ac.uk/id/eprint/4604/>

Document Version:

Article (Accepted Version)

---

The aim of the Leeds Beckett Repository is to provide open access to our research, as required by funder policies and permitted by publishers and copyright law.

The Leeds Beckett repository holds a wide range of publications, each of which has been checked for copyright and the relevant embargo period has been applied by the Research Services team.

We operate on a standard take-down policy. If you are the author or publisher of an output and you would like it removed from the repository, please [contact us](#) and we will investigate on a case-by-case basis.

Each thesis in the repository has been cleared where necessary by the author for third party copyright. If you would like a thesis to be removed from the repository or believe there is an issue with copyright, please contact us on [openaccess@leedsbeckett.ac.uk](mailto:openaccess@leedsbeckett.ac.uk) and we will investigate on a case-by-case basis.

**3D surface-imaging for volumetric measurement in people with obesity**

**Sean Clarkson<sup>1</sup>, Stuart W. Flint<sup>2</sup>, David R. Broom<sup>3</sup>, Matt Capehorn<sup>4</sup> and Jonathan Wheat<sup>3\*</sup>**

<sup>1</sup>Institute of Medical and Biological Engineering, School of Mechanical Engineering, University of Leeds, Leeds, United Kingdom, S.Clarkson@leeds.ac.uk

<sup>2</sup>School of Sport, Leeds Beckett University, Leeds, United Kingdom, S.W.Flint@leedsbeckett.ac.uk

<sup>3</sup>Academy of Sport and Physical Activity, Sheffield Hallam University, Sheffield, United Kingdom, D.R.Broom@shu.ac.uk, J.Wheat@shu.ac.uk

<sup>4</sup> Rotherham Institute for Obesity, Rotherham, United Kingdom, mcapehorn@yahoo.co.uk

\*Corresponding author

Jonathan Wheat

Academy of Sport and Physical Activity

Sheffield Hallam University

Sheffield

United Kingdom

S10 2BP

T: 0044 114 225 4330

F: 0044 114 225 4356

E: J.Wheat@shu.ac.uk

## **Abstract**

**BACKGROUND:** Current methods for tracking the progress of people with obesity towards a weight loss goal appear simple and potentially misleading. A technique to quantify change in body shape whilst visualising areas of the body where weight loss occurs would be advantageous, and has the potential to be used as a motivational tool. Three-dimensional (3D) surface-imaging would serve as a good basis for such a technique, however current systems are prohibitively expensive.

**OBJECTIVE:** Highlight the use of a cheaper alternative 3D surface-imaging system for volumetric measurement in people with obesity.

**METHODS:** A recently developed low-cost 3D surface-imaging system was used, having previously being validated in a healthy population. A total of 61 people with obesity, enrolled on a weight-loss programme, were surface-imaged using the system.

**RESULTS:** The findings suggest the low-cost system can obtain 3D surface-images of an obese human body, from which numerical parameters could be calculated and further analysis conducted.

**CONCLUSIONS:** Further studies will focus on the validity and reliability of such analyses and the potential of the system to be considered as a long-term instalment in primary healthcare settings as a weight loss aid.

Keywords: *3D Surface-imaging, Anthropometry, Obesity, Volume*

## **BACKGROUND**

Current methods to assess weight loss outcomes includes balance scales [1], tape measurement [1] or ‘before and after’ photographs [2]. These can mislead practitioners and patients, leading to inaccurate perceptions of effectiveness. For example, a patient may show no change in weight when stood on a balance scale, but may have lost weight from one area of the body whilst gaining weight elsewhere.

A measurement technique that enables change in body shape to be quantified, in addition to determining the areas of the body where change has occurred would enhance understanding of the impact and effectiveness of weight loss programmes. This technique would enable tracking of progress towards a weight loss goal, and could potentially be used as a motivational tool to encourage weight loss by enabling users to see how their body shape changes.

3D surface-imaging appears a suitable technique to measure body shape change. It reduces inaccuracies [3-4] inherent with current techniques, such as skin depression and soft tissue artefact [5] which is further exaggerated in people with obesity. 3D surface-imaging is less invasive than manual measurement and takes less time [6].

However, the majority of current 3D surface-imaging systems are prohibitively expensive (approximately £10,000) [7], require skilled operators, and involve lengthy post-processing of captured data. Wicke and Dumas [8] suggested structured light based systems would be a suitable low-cost alternative to current techniques. We have developed a low cost (~ £1,000) 3D surface-imaging system, comprising four pseudo structured light depth cameras (Microsoft Kinect<sup>®</sup>) capable of obtaining 3D surface-images of the human body in less than one second. However, thus far it has only been validated using a healthy weight population [9].

## **OBJECTIVE**

The objective of this technical paper is to highlight the use of the system when surface-imaging people with obesity. Future studies will focus on the development of techniques to obtain numerical parameters from the 3D surface-images.

## **METHODS**

### *The 3D Surface Imaging System*

The surface imaging system comprised four Microsoft Kinect<sup>®</sup> sensors mounted in a vertical orientation. This increased the vertical field of view, and allowed the Kinects<sup>®</sup> to be positioned closer to the people being scanned, maximising scan resolution [10].

Initial investigations suggested a capture area of 0.8m x 0.8m was sufficient to contain the range of participants that may be scanned. Kinects were affixed to tripods, located 1.75m from the centre of the capture area and 1.27m from the ground. Figure 1 shows the scanning system positioned in the Rotherham Institute for Obesity (RIO).

\*[Insert Figure 1 here]\*

Custom software created using the Microsoft Kinect<sup>®</sup> software development kit (Microsoft Corporation, Redmond, USA) was used to control the Kinects, perform calibration, and capture images. The Kinect's depth data can exhibit distortion, therefore each device was calibrated before first use [11].

The local coordinate system of each Kinect was aligned to a global frame, enabling capture of a single 3D model. A calibration object comprising four 120mm diameter spheres mounted on

a vertical rod was placed in nine positions covering the capture volume. Point clouds and corresponding depth images were captured by each Kinect. A technique comprising image processing, rigid body transformation [12], and RANSAC point discrimination [13] was used to produce the transformation matrices to align each point cloud with one another.

The entire calibration process (including data collection and processing) took approximately nine minutes. Once calibrated, bespoke software was used to capture 3D surface-images rendered with colour. The Kinect's infra-red (IR) projectors were switched on and off during capture, preventing interference between neighbouring sensors [13], resulting in a data collection time of around 0.9 seconds.

### **Participants**

After institutional ethical approval, 61 participants enrolled in RIO's programme were recruited. Participants read the information sheet and gave their consent. Inclusion criteria was a BMI > 30 kg/m<sup>2</sup> and able to stand unaided. Twenty-four of the participants were male, whilst thirty-seven were female. Other characteristics are summarised in Table 1.

\*[Insert Table 1 here]\*

### **Data Collection Protocol**

Participants were asked to remove their shirt, total body mass was recorded using a body composition analyser (Tanita, Amsterdam, Netherlands) and stature recorded using a Leicester height measure (Invicta Group, Leicester, United Kingdom).

Participants were palpated and marked with six coloured circular markers, identifying anatomical points in the colour mapped point clouds. Anterior markers were placed on the

xiphoid process and anterior superior iliac spine (ASIS). Posterior markers were placed over the spine at the same height as the anterior markers (Figure 2).

\*[Insert Figure 2 here]\*

Footprints were placed on the floor to ensure participants stood in the correct place during capture. The position and orientation of the footprints was designed to aid balance and reduce postural sway, improving scan reliability [9].

Participants were asked to adopt the ISO 20685-1 [14] scanning pose, with arms abducted by 20° with respect to their trunk. However, this led to areas of the point cloud being occluded or merged together, owing to the size of participants' arms so the pose was adapted, to an abduction angle of 75°. Hand supports (tripods) were used to limit involuntary movement during scanning by providing light touch stabilisation [15-16], and to assist reliably adopting the same position.

Participants were asked to hold their breath at the end of the expiration cycle (end-tidal expiration) throughout the imaging [6]. This ensured the diaphragm was empty, limiting shape change of the trunk between data capture, aiding reliability.

Three-point clouds of each participant were collected, with the participant leaving and re-entering the capture area between each collection. The field of view was restricted so that little more than the torso segment was included to ensure each participant was anonymised.

## **Results and Discussion**

Each point cloud was visually inspected to determine data quality. Each point cloud successfully captured a 3D surface profile of the participant's torso segment (Figure 3).

\*[Insert Figure 3 here]\*

Point clouds of some participants were found to contain holes (Figure 4) around the spine and lower abdomen.

\*[Insert Figure 4 here]\*

Holes around the abdomen were caused by areas being occluded from the Kinects by excess or overhanging fat and skin. Holes around the spine were caused by participants having a more prominent surface profile to the left and right of their spine - due to their large body mass, occluding this area from the Kinect's view. This problem could be reduced by making the spinal area more prominent to one of the sensors but issues could arise in other areas of the body. Importantly, the physical size of such gaps in the surface were not a problem, and could be cleaned using available 3D hole filling algorithms and smoothing splines.

Difficulties were encountered when palpating and marking some participants. For example, it wasn't possible to accurately palpate and mark the ASIS points on participants with large amounts of overhanging fat and skin around the lower stomach, as bony landmarks weren't apparent. Excess fat and skin means the markers will likely move around between imaging, and are unlikely to accurately represent their intended points under the skin, impacting inter-scan reliability. Little can be done to adapt the land-marking protocol to reduce these problems in people with obesity.

It was not possible to use the ISO 20685-1 scanning pose, owing to the size of participants arms and overlap with the trunk. Given the increased abduction angle used in this study (75° instead of 25°), there is greater potential for movement of skin and tissue, potentially reducing inter-scan reliability. Hand supports are needed to ensure participants adopt the same scanning position over repeated scans.

Owing to reduced mobility and larger size of some participants, there was a greater likelihood of the system being knocked when participants entered and exited the scanning area. Therefore, the system was recalibrated between each participant. This was only a requirement due to Kinect® sensors being mounted on tripods which would not be necessary if the system was permanently installed.

### **Conclusion**

Our low-cost 3D surface-imaging system can be used to capture 3D surface profiles of people with obesity, is the first attempt to do so, and we have developed a protocol to optimise inter-scan reliability and surface accuracy. Holes were found in the surface data of some participants, owing to their individual physique. However, these could be eliminated with simple post-processing techniques. Future studies should focus on extracting measurements from the 3D surface data, quantifying inter-scan reliability, and demonstrating feasibility of this measurement in primary healthcare settings. Research should also seek to assess suitability of the system for motivating and quantifying weight loss.

### **Acknowledgements**

The authors would like to thank all the participants for taking part in this research. We would like to thank Charlotte Simpson with assistance with data collection and the Rotherham Institute for Obesity for use of their premises and support with the project.

### **Authors' contributions**

SC, SF, DB and JW were involved in the conception and design of the study. SF and SC conducted the literature review. MC provided access to the participants. SC undertook the data collection. SC & JW analysed and interpreted the data. SC and SF drafted the manuscript. SC, SF, DB, MC and JW were involved in revising the manuscript and finalising the content of the manuscript. All authors read and approved the final manuscript.

### **References**

1. National Heart Blood and Lung Institutes. Clinical Guidelines on the Identification, Evaluation, and Treatment of Overweight and Obesity in Adults, *National Heart, Lung, and Blood Institute*. 1998. <http://www.ncbi.nlm.nih.gov/books/NBK2009/> (last accessed November 21, 2017).
2. Daly A. Can Selfies Help You Lose Weight? *Women's Health*. 2013. <http://www.womenshealthmag.com/weight-loss/fitness-motivation-pictures> (last accessed November 21, 2017).
3. Durkin JL, Dowling JJ, Andrews DM. The measurement of body segment inertial parameters using dual energy X-ray absorptiometry. *J Biomech*. 2002; 35(12): 1575–80.
4. Wan Y, Hu G, Dong G. Anthropometric techniques based on kinect 3D scanning. In *International Conference on Mechatronic Sciences, Electric Engineering and Computer*. 2013. Shenyang, China.
5. O'Haire C, Gibbons P. Inter-examiner and intra-examiner agreement for assessing sacroiliac anatomical landmarks using palpation and observation: pilot study. *Manual Ther*. 2000; 5(1): 13-20.
6. Schranz N, Tomkinson G, Olds T, Daniell N. Three-dimensional anthropometric analysis: differences between elite Australian rowers and the general population. *J Sport Sci*. 2010; 28(5): 459–69.
7. Weiss A, Hirshberg D, Black MJ. Home 3D Body Scans from Noisy Image and Range Data. In *13th International Conference on Computer Vision*. 2011. Barcelona, Spain.
8. Wicke J, Dumas GA. Influence of the Volume and Density Functions Within Geometric Models for Estimating Trunk Inertial Parameters. *J App Biomech*. 2010; 26: 26–31.
9. Clarkson S, Wheat J, Heller B, Choppin S. Assessing the Suitability of the Microsoft Kinect for Calculating Person Specific Body Segment Parameters. In *4th IEEE Workshop on*

- Consumer Depth Cameras for Computer Vision, European Conference on Computer Vision*. 2014. Zurich, Switzerland: IEEE.
10. Khoshelham K, Elberink SO. Accuracy and resolution of Kinect depth data for indoor mapping applications. *Sensors*. 2012; 12(2): 1437–54.
  11. Clarkson S, Wheat J, Heller B, Webster J, Choppin S. Distortion Correction of Depth Data from Consumer Depth Cameras. In Hometrica Consulting, ed. *3D Body Scanning Technologies*. 2013. Long Beach, California: Hometrica Consulting, pp. 426–437.
  12. Challis JH. A procedure for determining rigid body transformation parameters. *J Biomech*. 1995; 28(6): 733–737.
  13. Clarkson S, Choppin S, Hart J, Heller B, Wheat J. Calculating Body Segment Inertia Parameters from a Single Rapid Scan Using the Microsoft Kinect. In Hometrica Consulting, ed. *3D Body Scanning Technologies*. 2012. Lugano, Switzerland: Hometrica Consulting, pp. 153–163.
  14. International Standards Office, 2010. *ISO 20685, 3-D Scanning Methodologies for Internationally Compatible Anthropometric Databases* 2010. <http://www.iso.org/iso> (last accessed November 21, 2017).
  15. Kouzaki M, Masani K. Reduced postural sway during quiet standing by light touch is due to finger tactile feedback but not mechanical support. *Exp Brain Res*. 2008; 188(1): 153–8.
  16. Lackner J, Rabin E, DiZio P. Stabilization of posture by precision touch of the index finger with rigid and flexible filaments. *Exp Brain Res*. 2001; 139(4): 454–464.
  17. Clarkson S, Wheat J, Heller B, Choppin S. Assessment of a Microsoft Kinect-based 3D scanning system for taking body segment girth measurements: a comparison to ISAK and ISO standards. *J Sport Sci*. 2016; 34(11): 1006-1014.

**Table 1: Summary characteristics of participants (n = 61)**

	<b>Mean</b>	<b>Standard Deviation</b>
<b>Age (years)</b>	46	14
<b>Mass (kg)</b>	114.2	24.3
<b>Stature (m)</b>	1.7	0.1
<b>BMI (kg/m<sup>2</sup>)</b>	40.4	6.1

## Figure Captions

**Figure 1:** Physical layout of the scanning system at the Rotherham Institute for Obesity.

**Figure 2:** Location of the anatomical markers. Five markers were attached: 1) Xiphoid process, 2) Left ASIS, 3) Right ASIS, 4) spine, at the height of the ASIS markers, 5) spine, at the height of the Xiphoid marker.

**Figure 3:** A typical 3D surface image from the system.

**Figure 4:** Holes in the returned 3D surface data.

## RUNNING HEAD: 3D SURFACE IMAGING



Figure 1

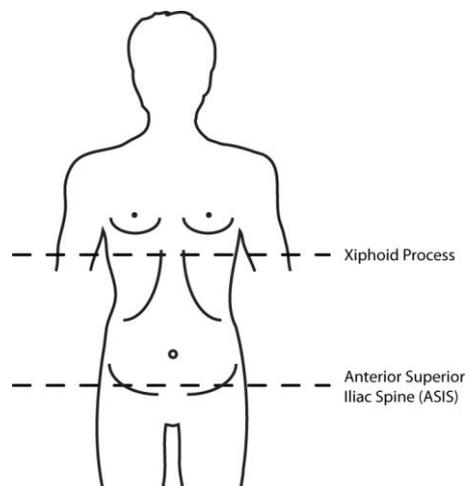


Figure 2



Figure 3

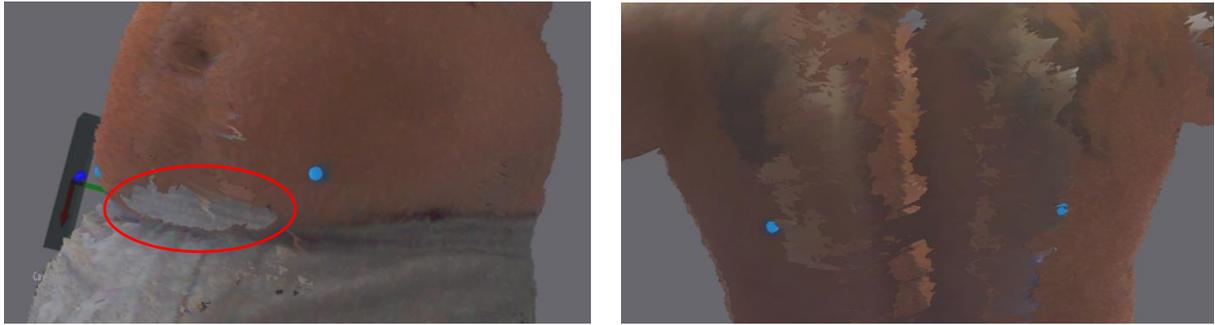


Figure 4

